


002127 8.1.1.5.150

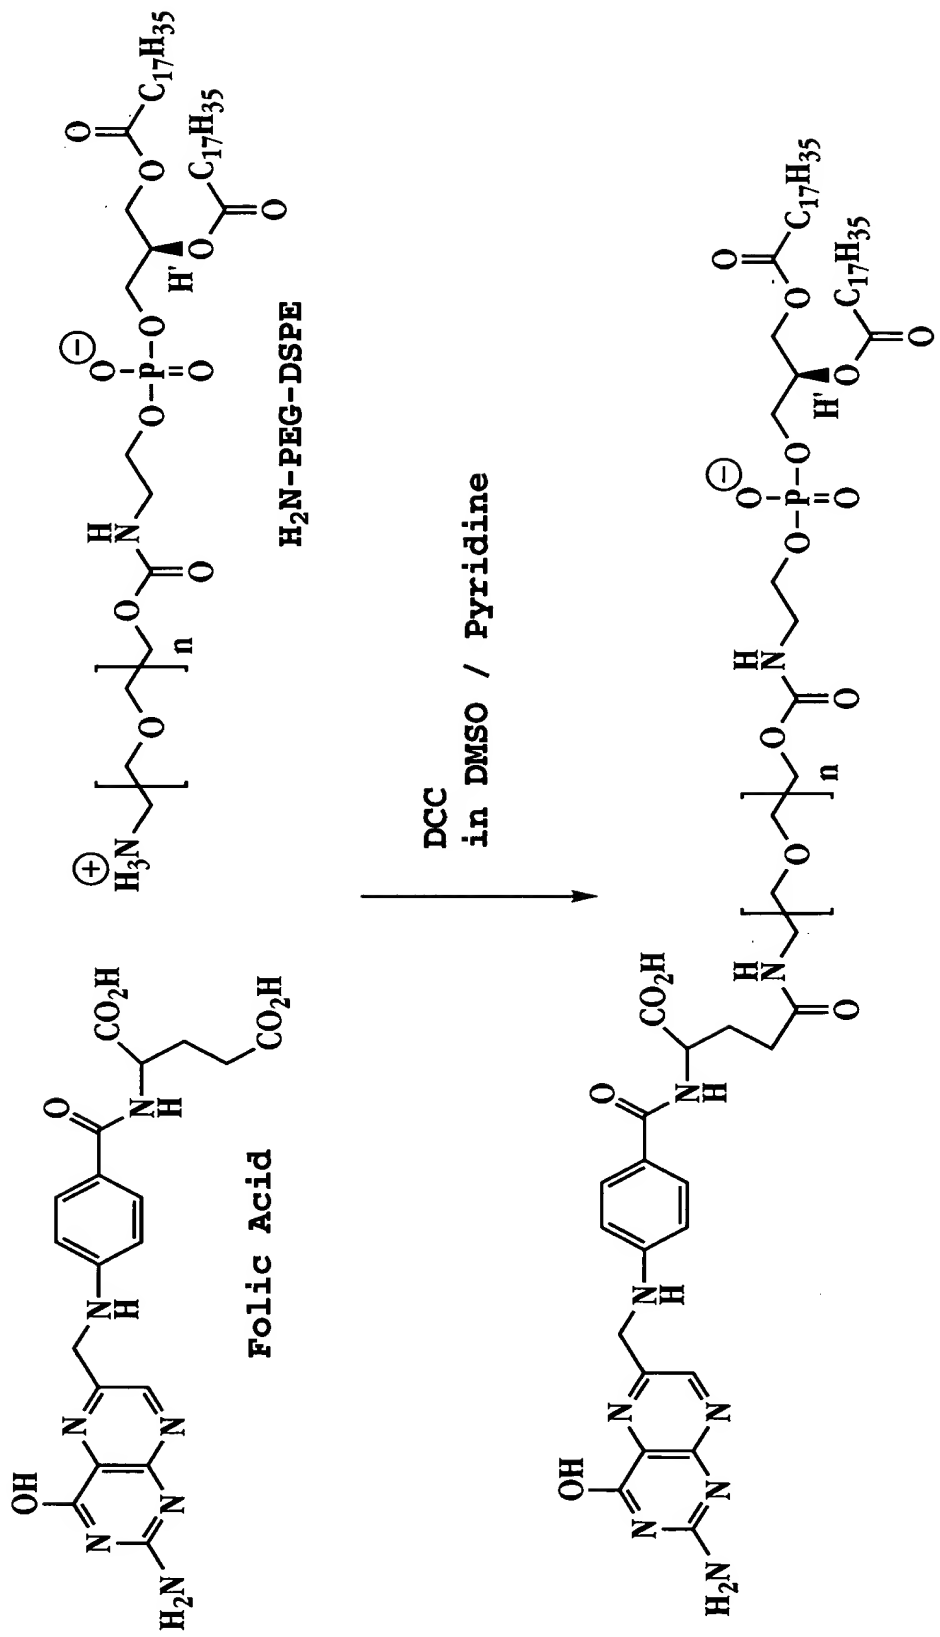

**Fig. 1**

APPROVED	G.G. FIG.	
BY	CLASS	SUBCLASS
DRAFTSMAN		

66272T "CTH29460



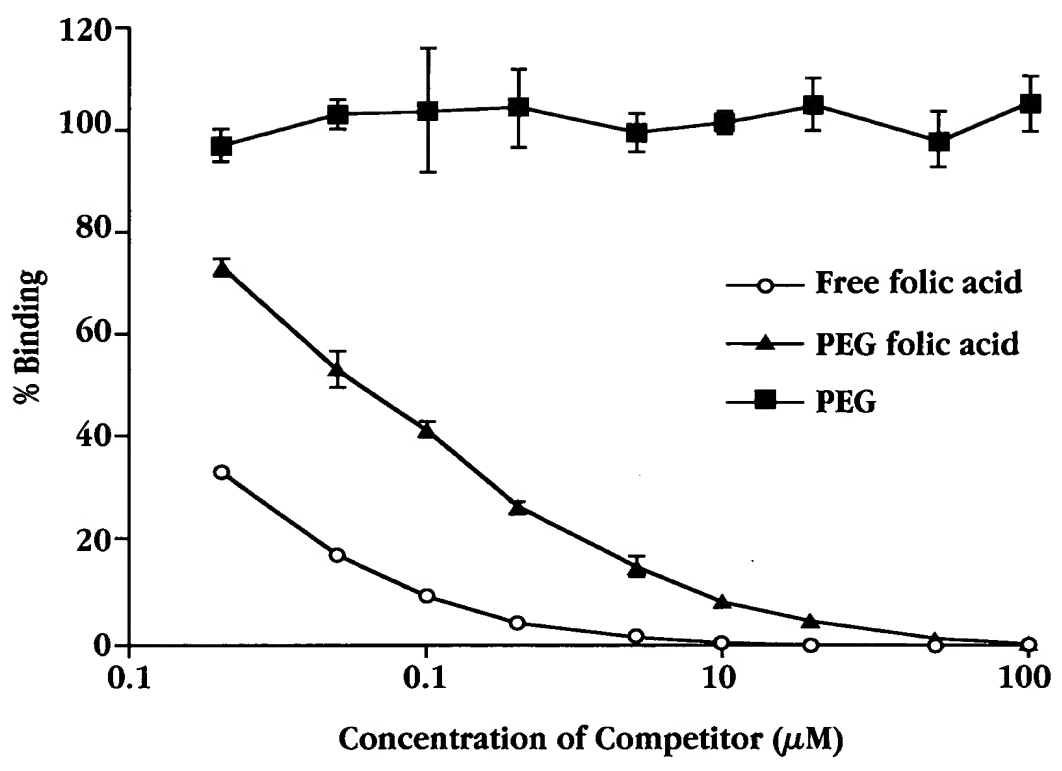


Fig. 2




Low mPEG2000

**Fig. 3A**




FA-PEG2000

**Fig. 3B**

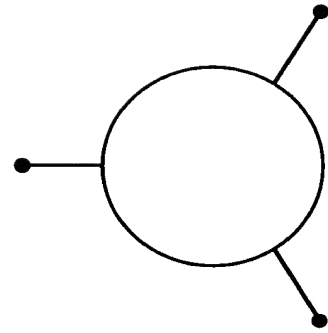


FA-PEG3350

**Fig. 3C**

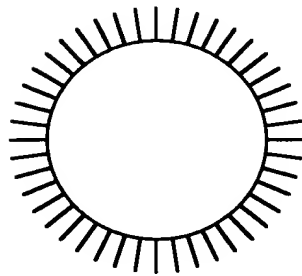


High mPEG2000

**Fig. 3D**

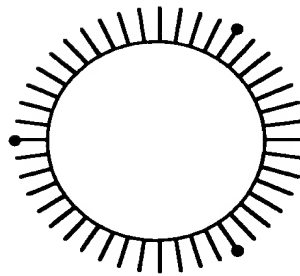


FA-PEG2000/mPEG

**Fig. 3E**

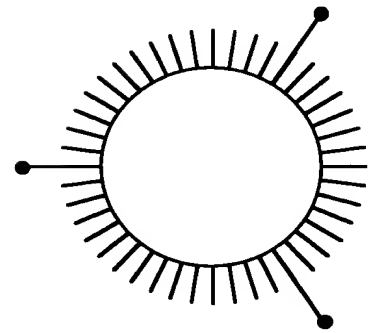


FA-PEG3350/mPEG

**Fig. 3F**

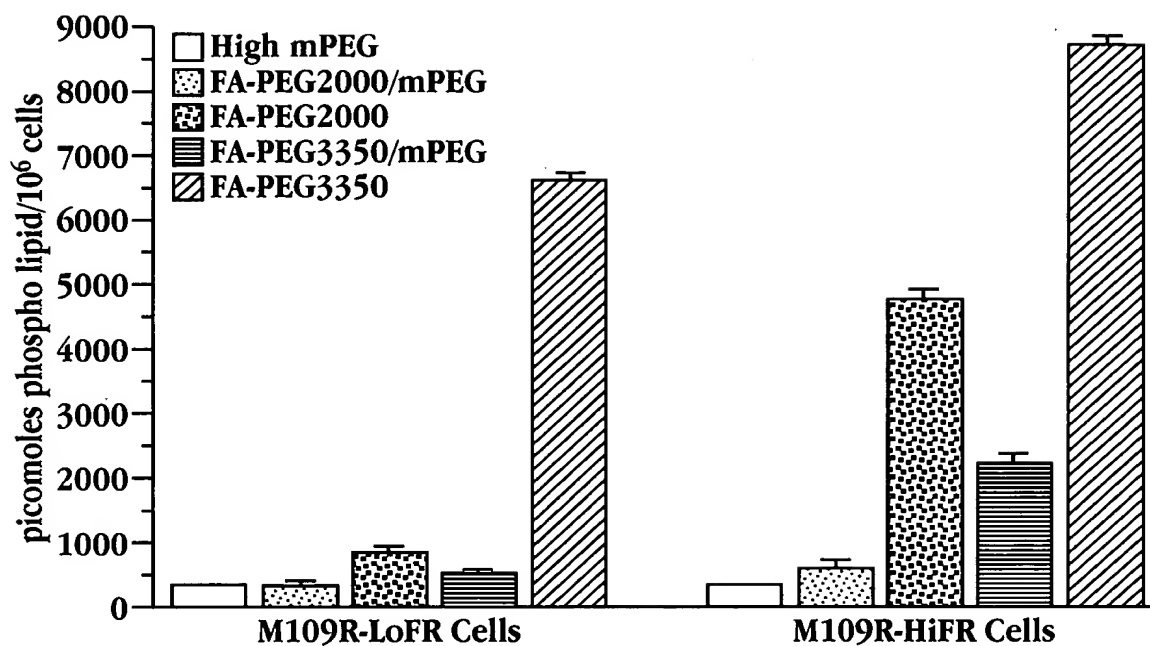


**Fig. 4A**

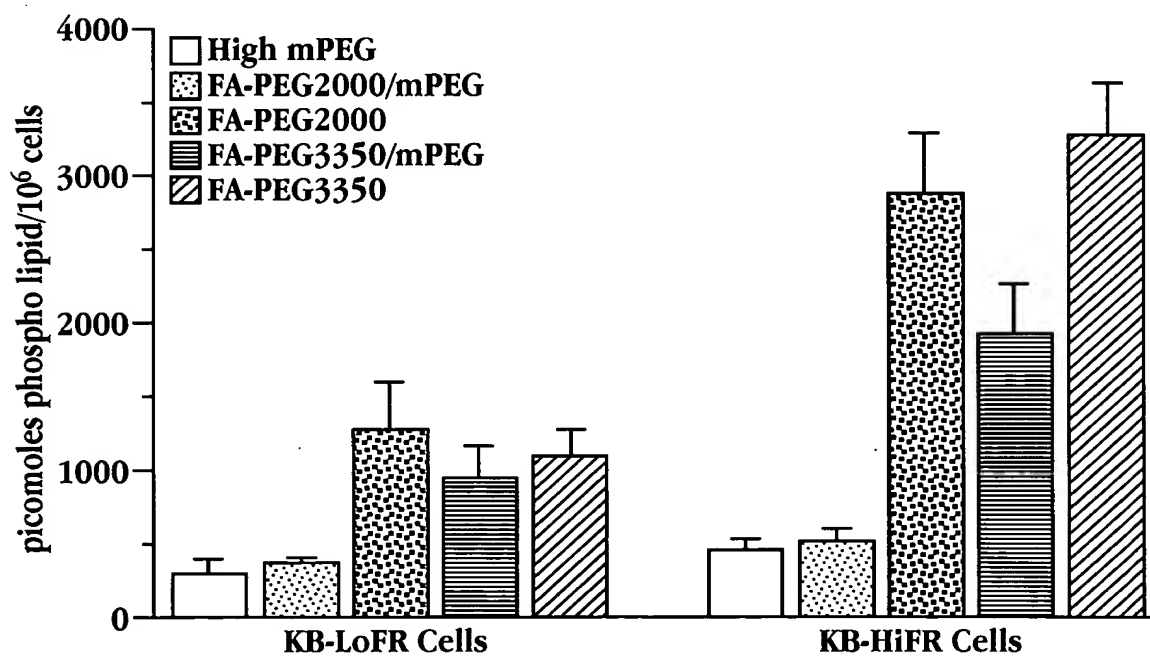

**Fig. 4B**

**Fig. 5A**

**Fig. 5B**

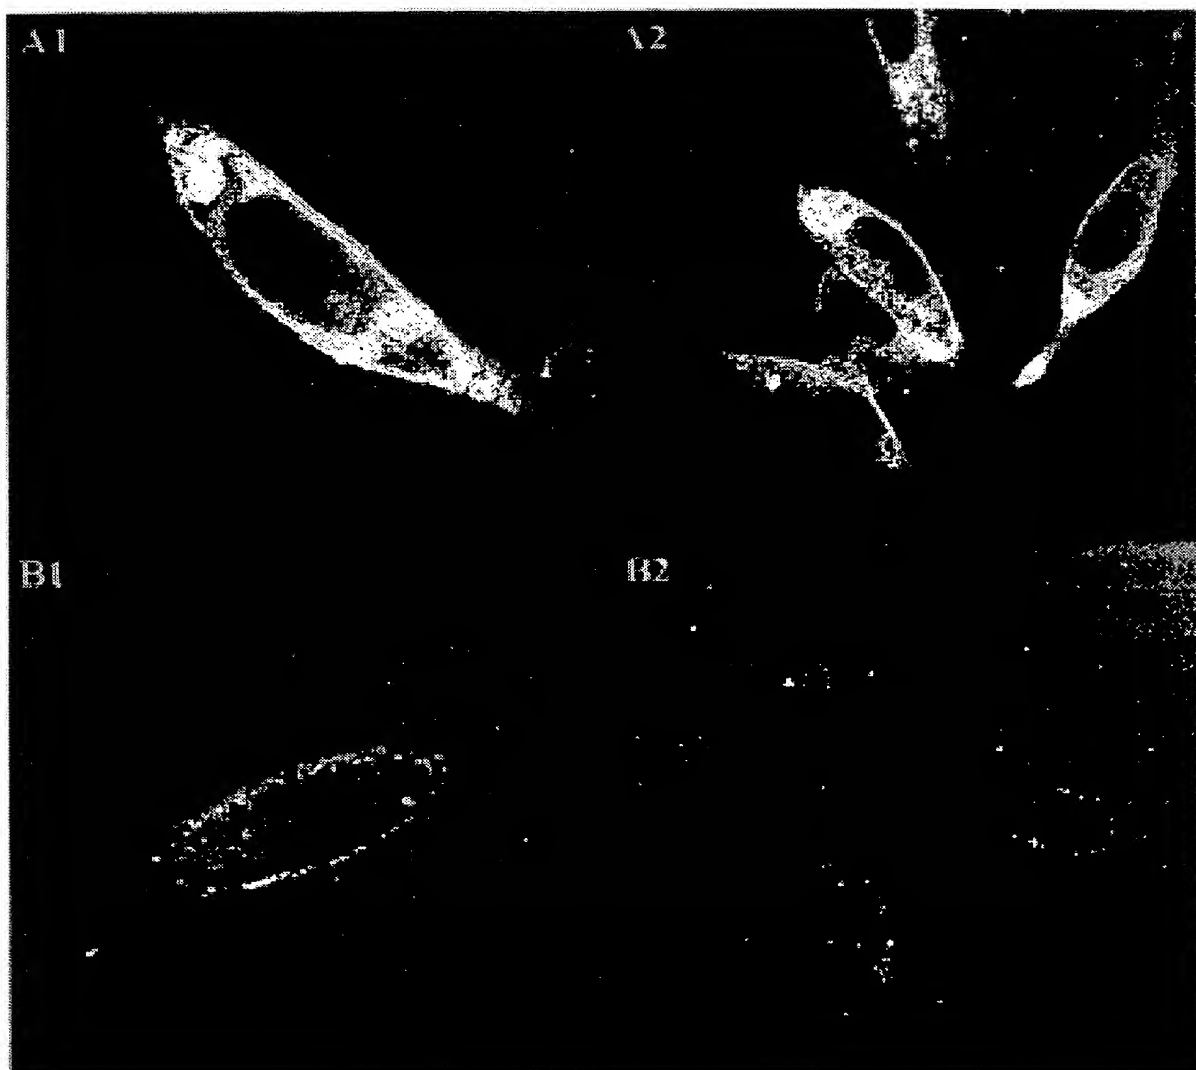


**Fig. 5C**

**Fig. 5D**

09467413 121799  
662727 ETHZ9460

09467413-124739  
66727 ET 4/9/60

**Fig. 6A**

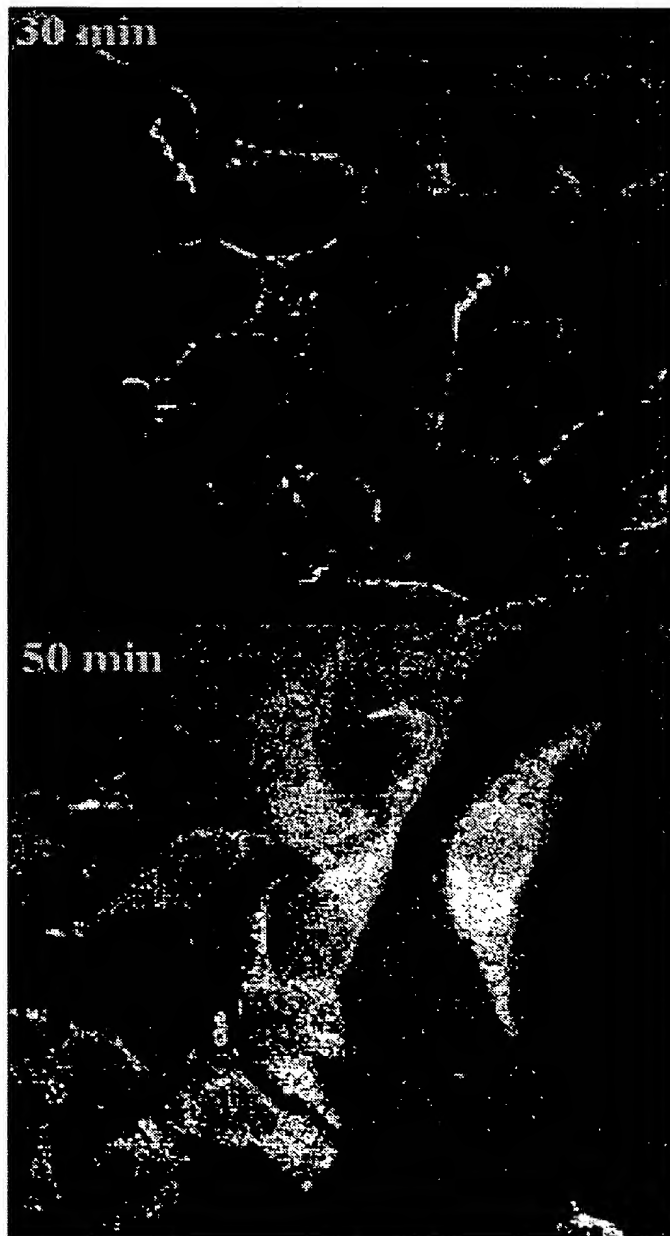

**Fig. 6B**


09467413 121799

**Fig. 7A**



**Fig. 7B**

662727" E F 429460

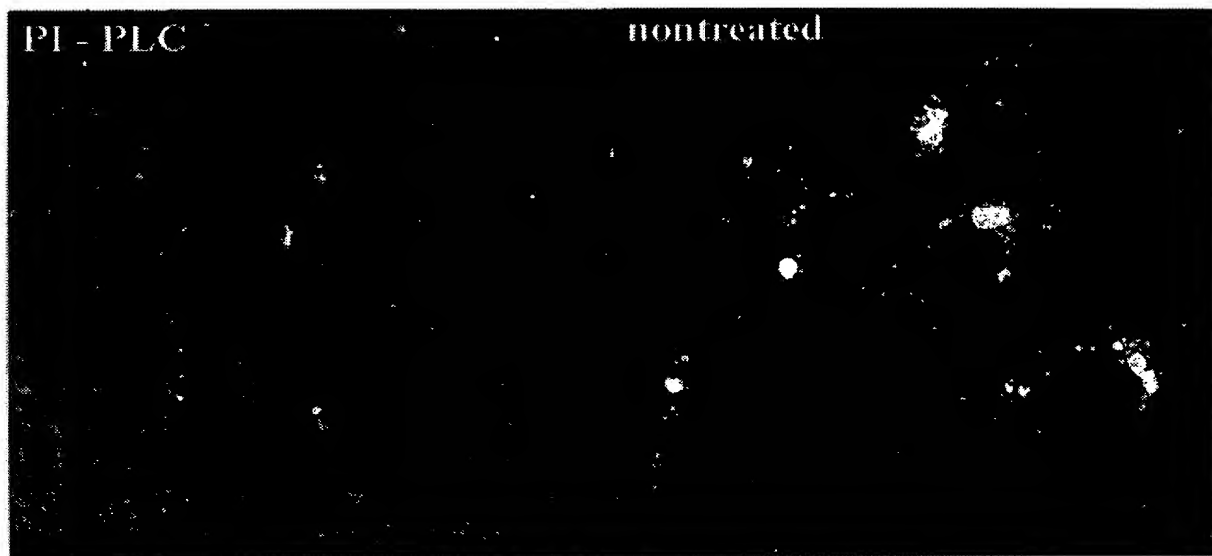


**Fig. 8A**

**Fig. 8B**




FreeDOX - 7min

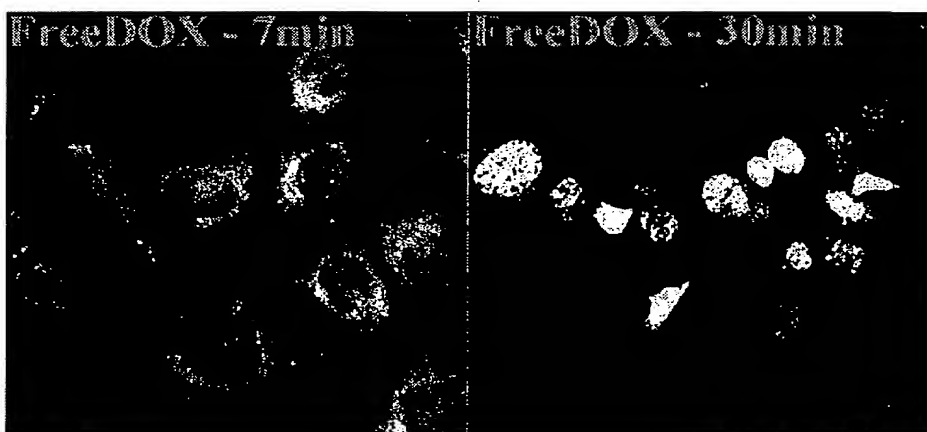


**Fig. 9A**

FreeDOX - 30min

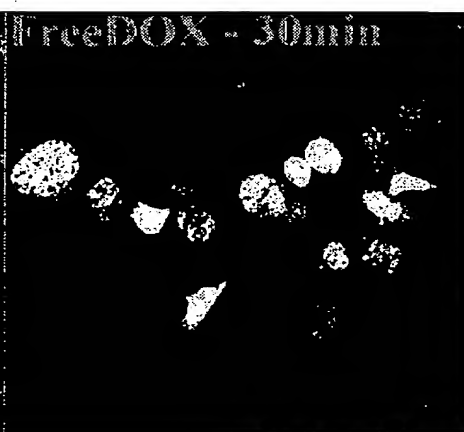

**Fig. 9B**

LipoDOX - 20min

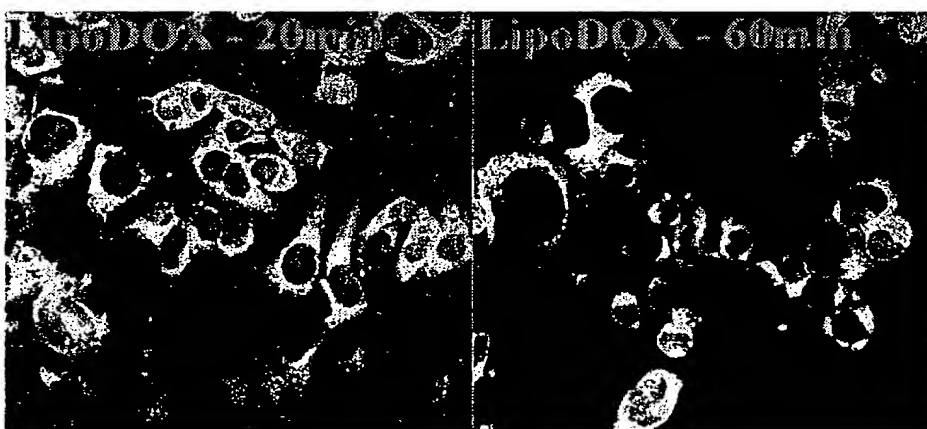


**Fig. 9C**

LipoDOX - 60min



**Fig. 9D**

LipoDOX - 90min

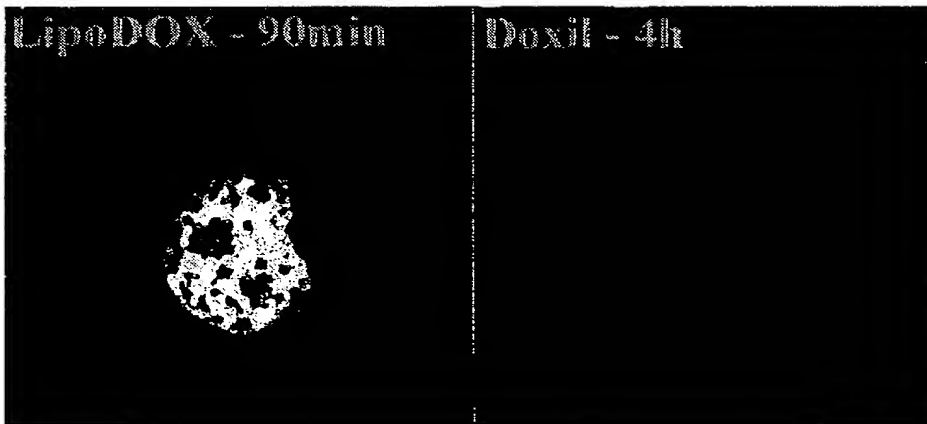


**Fig. 9E**

Doxil - 4h




**Fig. 9F**

0946743-1279  
65/ET-ET-9460

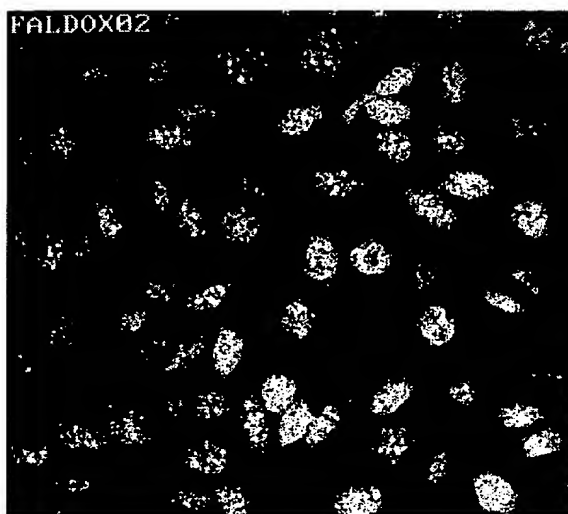

**Fig. 10A**

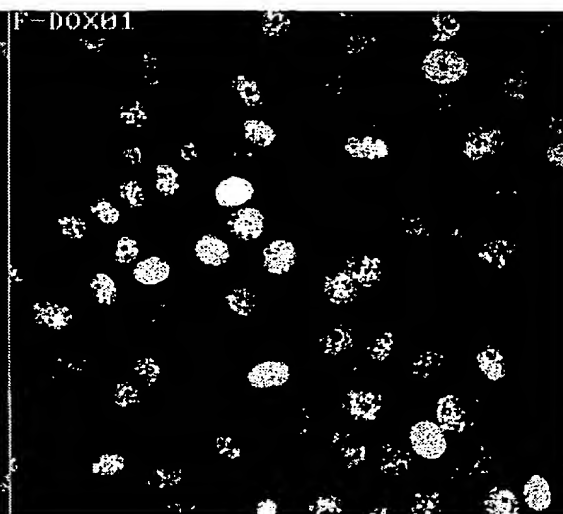


**Fig. 10B**




**Fig. 10C**


**Fig. 10D**

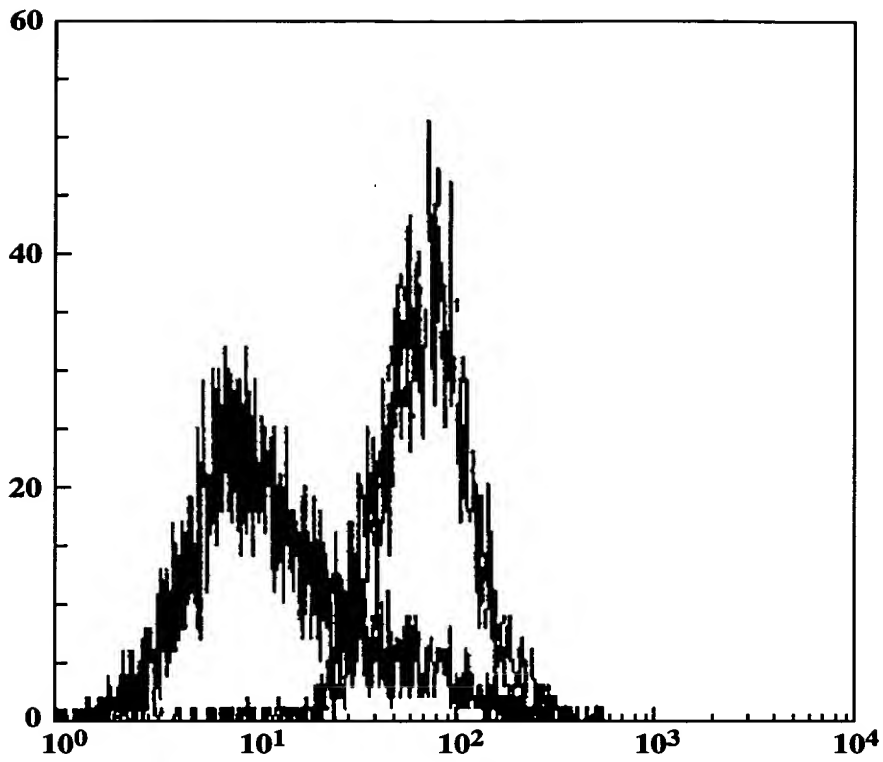


**Fig. 11A**

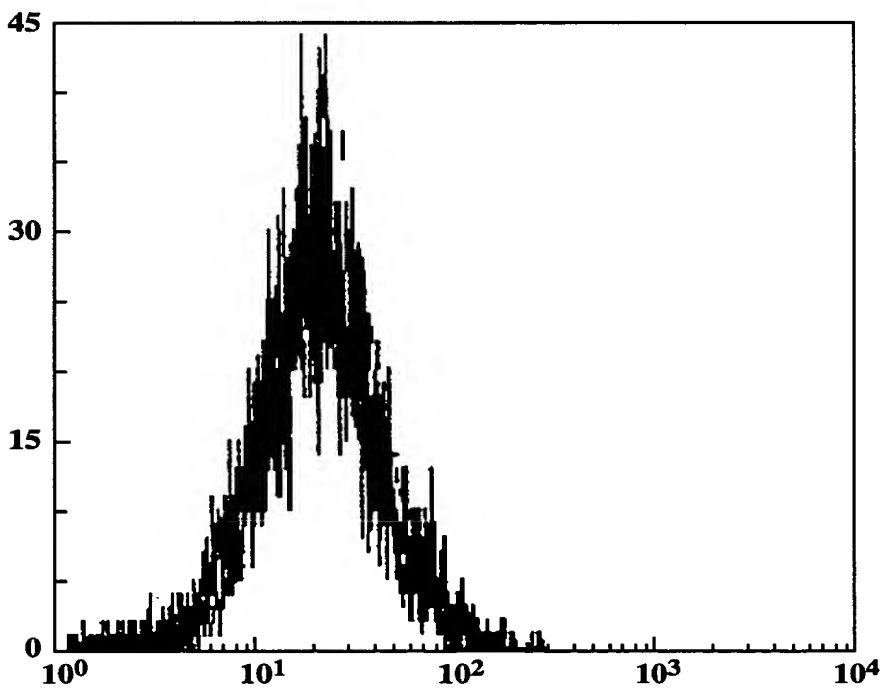

**Fig. 11B**

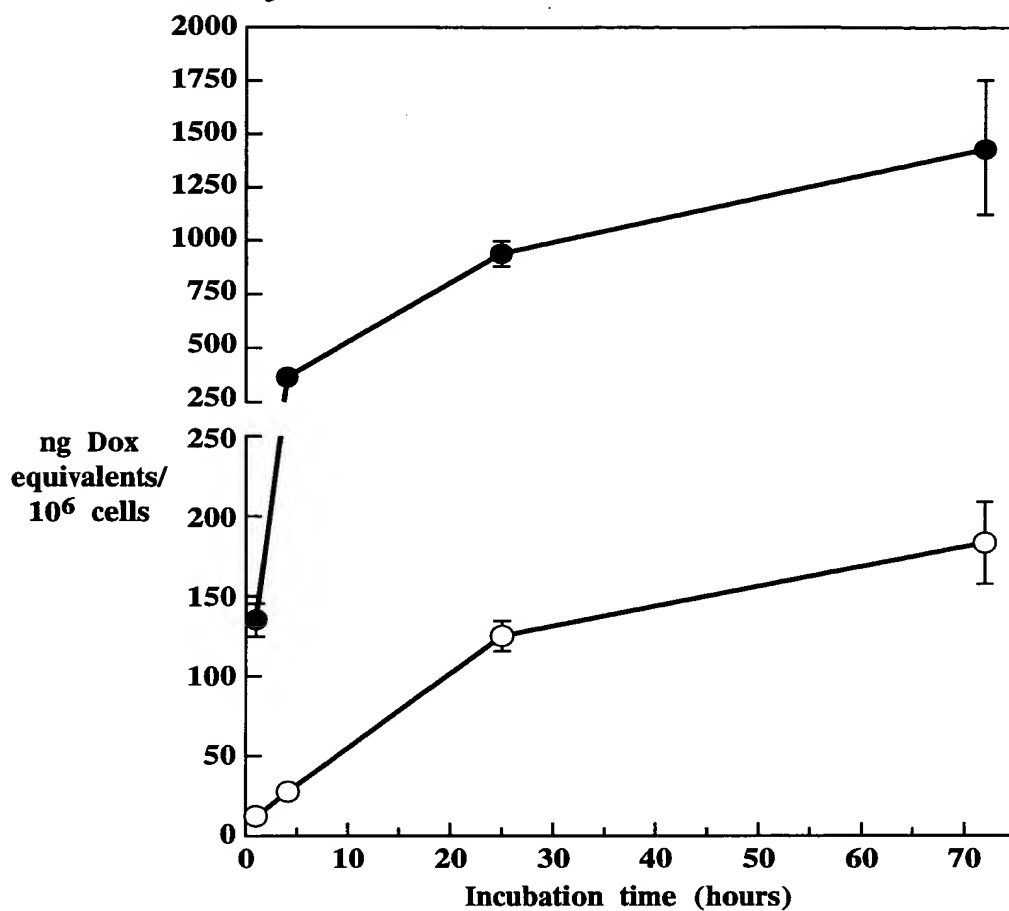

**Fig. 12**

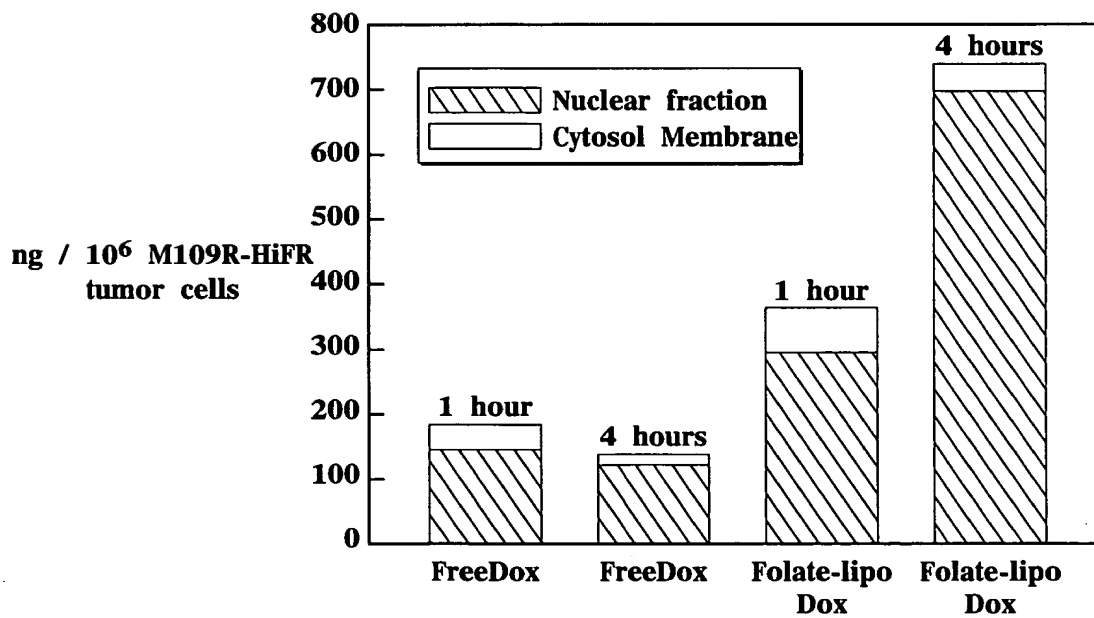

**Fig. 13**

09467443 124799

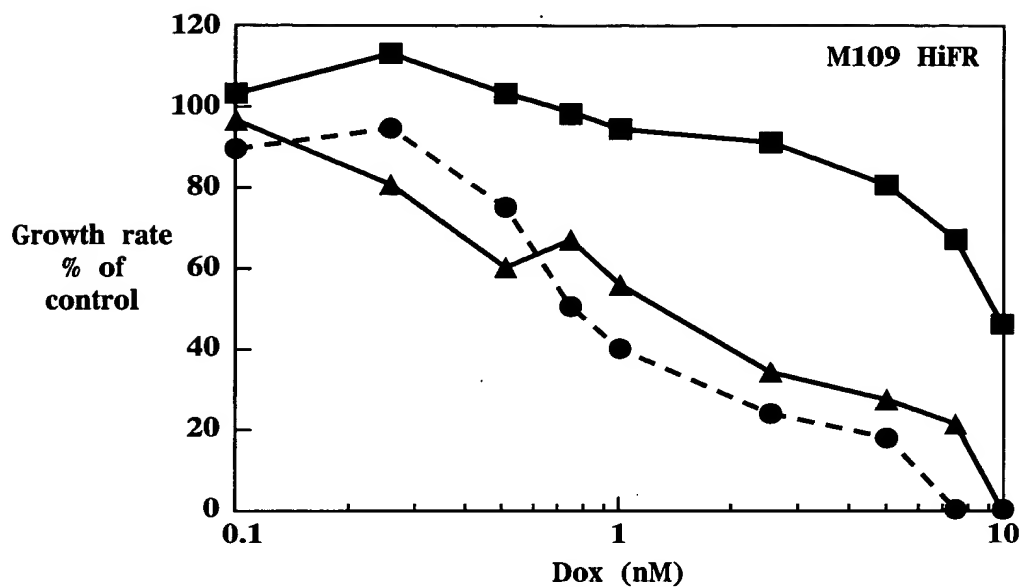


Fig. 14A


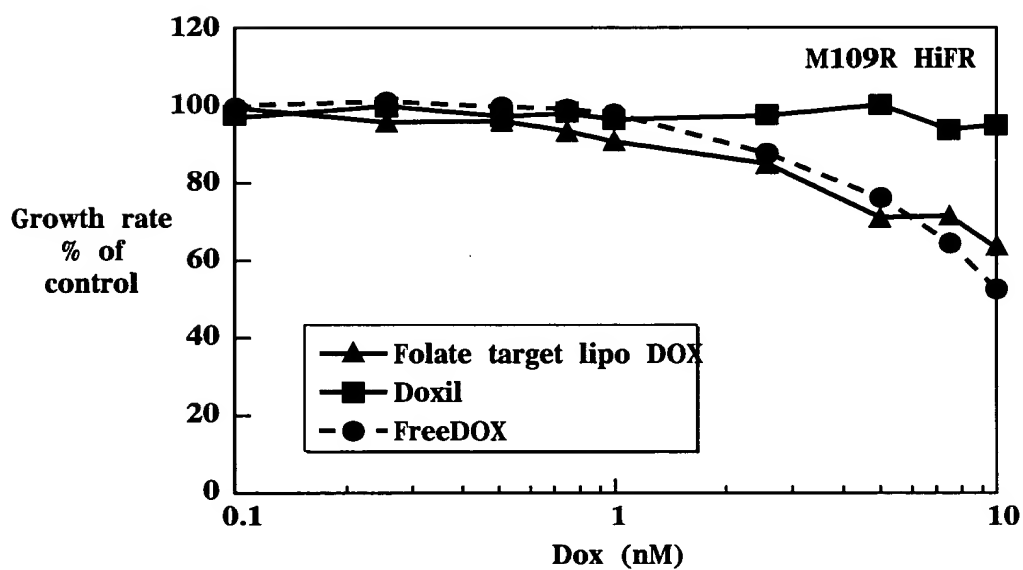


Fig. 14B



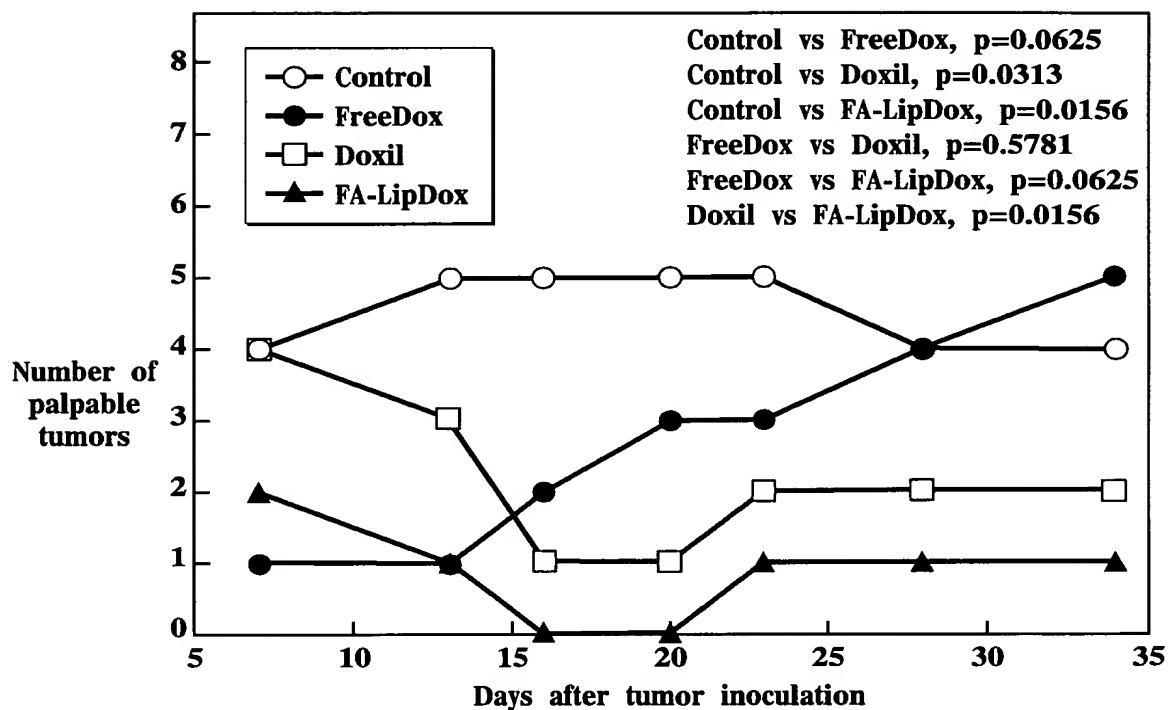

**Fig. 16**